

1H spectrum

Current Data Parameters
NAME mf_24_252
EXPNO 8
PROCNO 1


F2 - Acquisition Parameters
Date_ 20240718
Time_ 14.28
INSTRUM gn500
PROBHD 5 mm broadband
PULPROG zg30
TD 81728
SOLVENT CDCl3
NS 8
DS 2
SWH 8012.820 Hz
FIDRES 0.098043 Hz
AQ 5.0998273 sec
RG 161.3
DW 62.400 usec
DE 6.00 usec
TE 298.0 K
D1 0.10000000 sec
MCREST 0 sec
MCWRK 0.01500000 sec

==== CHANNEL f1 =====
NUC1 1H
P1 12.00 usec
PL1 -6.00 dB
SFO1 498.4534891 MHz

F2 - Processing parameters
SI 65536
SF 498.4500303 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

7.26

3.59
3.58
3.56
3.56
3.55
3.53
1.95
1.93
1.92
1.76
1.75
1.74
1.74
1.73
1.72
1.60
1.58
1.58
1.47
1.44
1.43
1.43
1.42
1.42
1.41
1.40
1.39
1.39
1.38
1.37
1.31
1.30
1.29
1.27
1.27
1.25
1.25
1.24
1.23
1.22
1.21
1.14
1.13
1.11
1.11
1.09
1.09

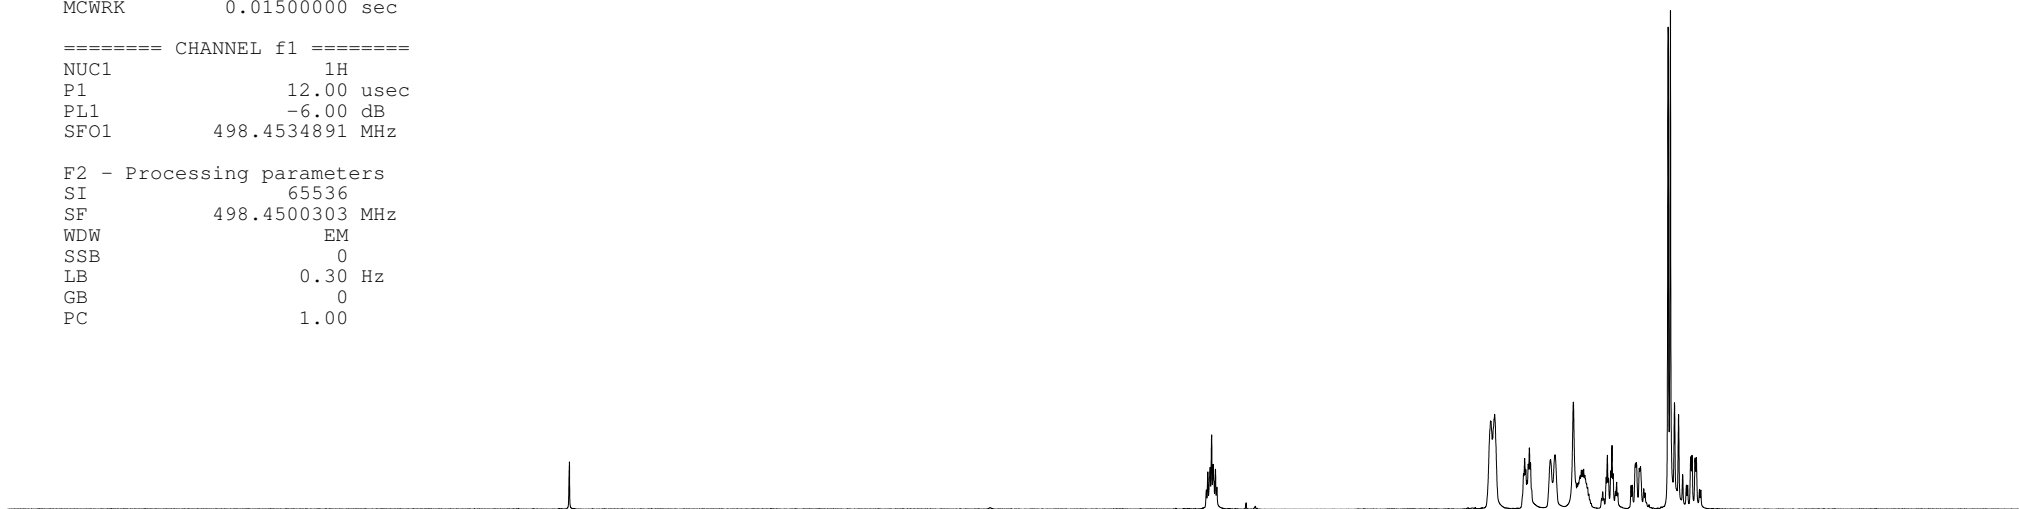

10 9 8 7 6 5 4 3 2 1 0 ppm

0.97
1.98
1.03
1.03
1.94
1.07
1.02
2.94
1.05
1.02