

1H spectrum

1.95
1.95
1.93
1.92

1.76
1.75
1.74
1.74
1.73
1.72
1.72

1.60
1.58
1.47
1.44
1.43
1.43
1.42
1.42
1.41
1.40
1.40
1.39
1.39
1.38
1.37
1.31
1.30
1.29
1.27
1.27
1.25
1.25
1.24
1.23
1.22
1.21
1.14
1.13
1.11
1.11
1.09
1.09
1.08
1.06
1.06

0.92
0.91
0.89
0.86
0.84
0.79
0.79
0.77
0.76
0.74
0.74

Current Data Parameters

NAME mf_24_252
EXPNO 8
PROCNO 1

F2 - Acquisition Parameters


Date_ 20240718
Time 14.28
INSTRUM gn500
PROBHD 5 mm broadband
PULPROG zg30
TD 81728
SOLVENT CDCl3
NS 8
DS 2
SWH 8012.820 Hz
FIDRES 0.098043 Hz
AQ 5.0998273 sec
RG 161.3
DW 62.400 usec
DE 6.00 usec
TE 298.0 K
D1 0.10000000 sec
MCREST 0 sec
MCWRK 0.01500000 sec

==== CHANNEL f1 =====

NUC1 1H
P1 12.00 usec
PL1 -6.00 dB
SFO1 498.4534891 MHz

F2 - Processing parameters

SI 65536
SF 498.4500303 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

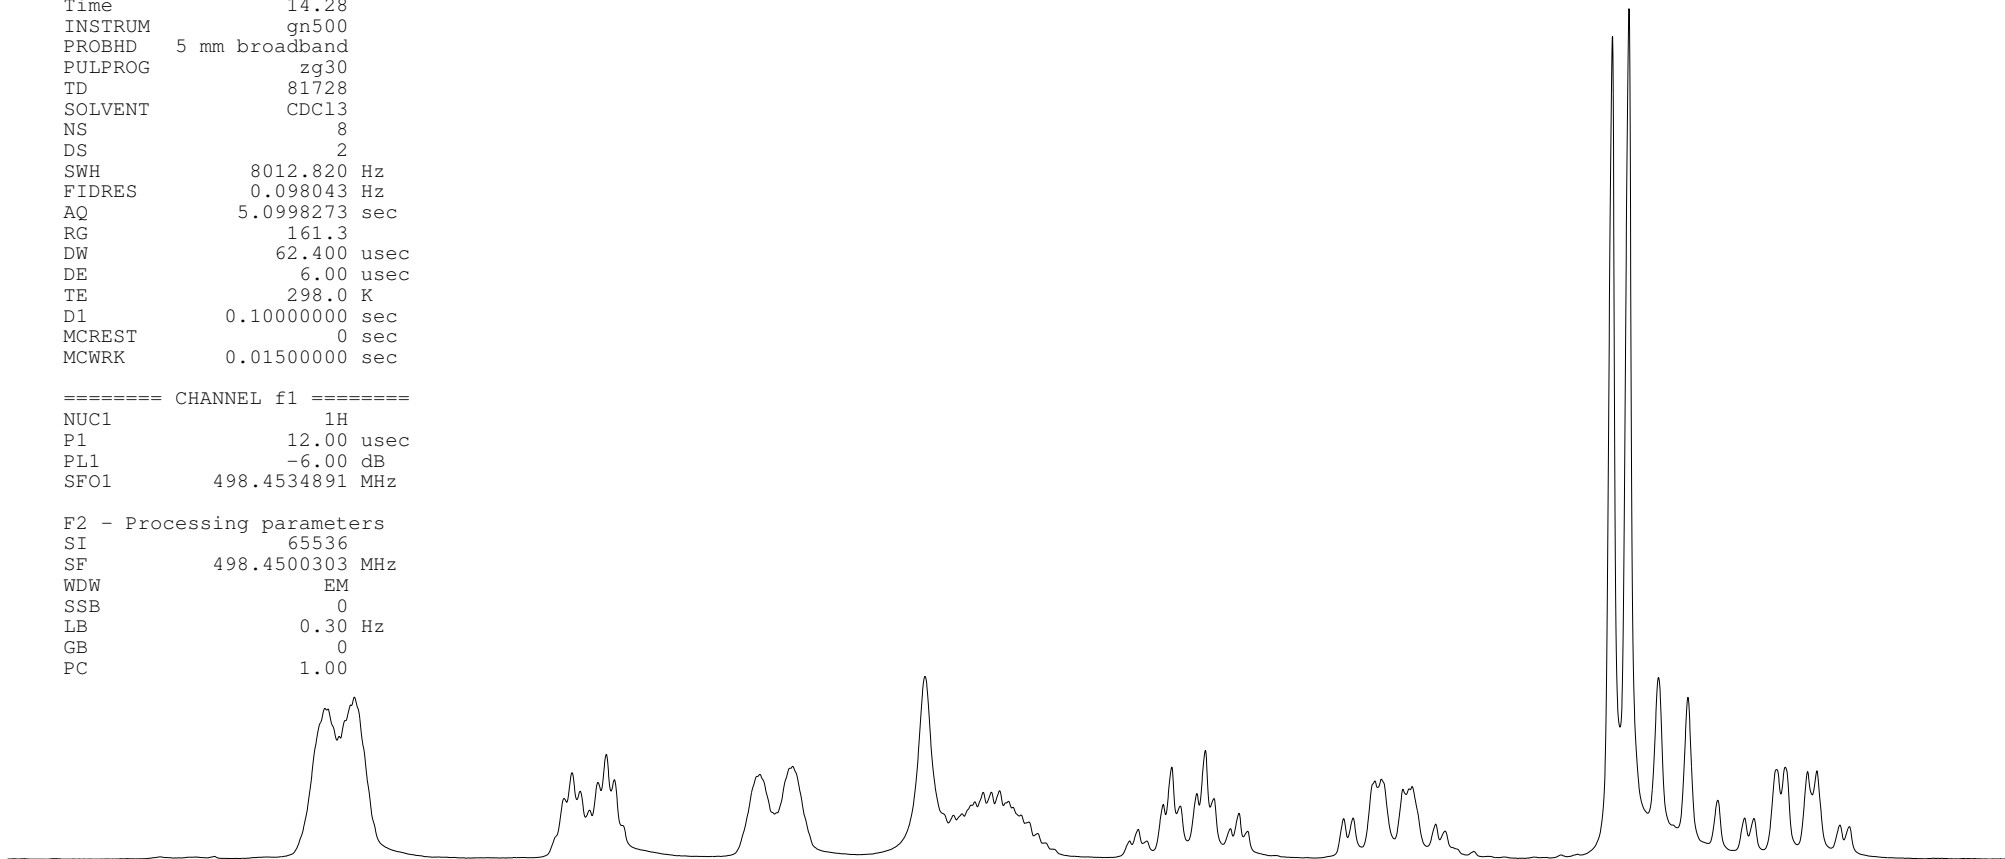

2.1 2.0 1.9 1.8 1.7 1.6 1.5 1.4 1.3 1.2 1.1 1.0 0.9 0.8 0.7 ppm

1.98

1.03

1.03

1.94

1.07

1.02

2.94

1.05

1.02