

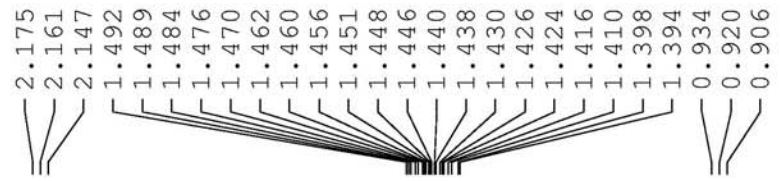
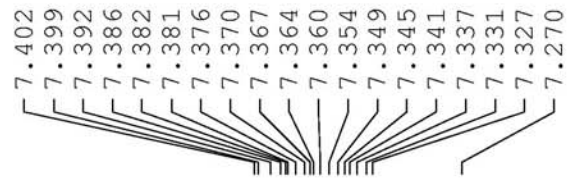


tp OS 3-5-37 1H CDC13 nmr500 4/27/07

Current Data Parameters  
NAME tp OS 3-5-37  
EXPNO 1  
PROCNO 1


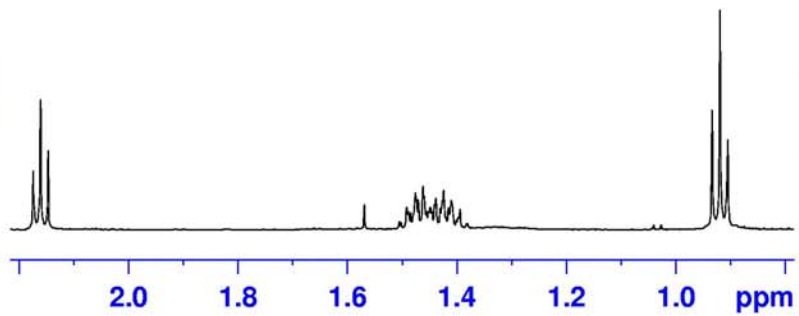


F2 - Acquisition Parameters:  
Date\_ 20070427  
Time 12.46  
INSTRUM spect  
PROBHD 5 mm Multinucl  
PULPROG zg  
TD 65536  
SOLVENT CDC13  
NS 10  
DS 2  
SWH 10330.578 Hz  
FIDRES 0.157632 Hz  
AQ 3.1719923 sec  
RG 32  
DW 48.400 usec  
DE 6.00 usec  
TE 298.2 K  
D1 10.00000000 sec  
TD0 1

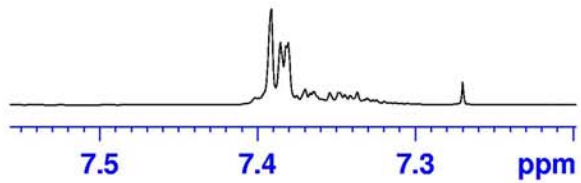

==== CHANNEL f1 =====  
NUC1 1H  
P1 9.00 usec  
PL1 0.00 dB  
SFO1 500.1330885 MHz

F2 - Processing parameters  
SI 32768  
SF 500.1300082 MHz  
WDW EM  
SSB 0  
LB 0.10 Hz  
GB 0  
PC 1.00

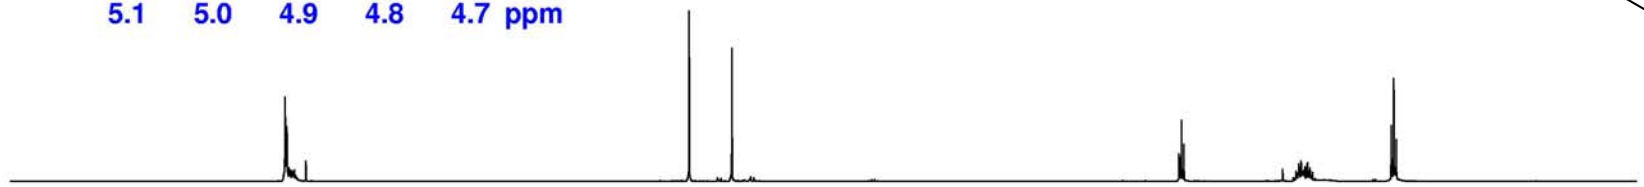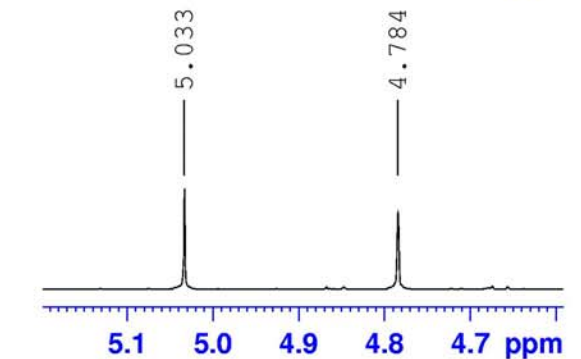

5.07

1.85

1.83

1.85

3.99

3.00

