
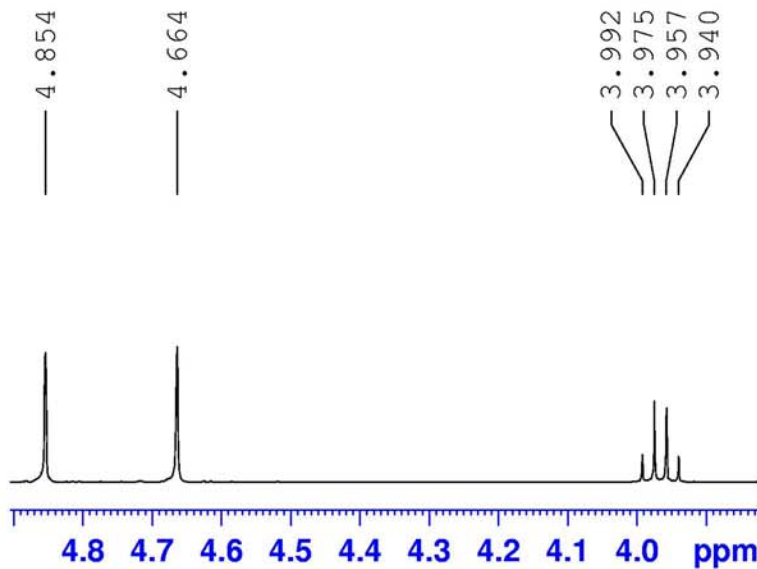


Current Data Parameters  
 NAME tp OS 2-5-36  
 EXPNO 1  
 PROCNO 1

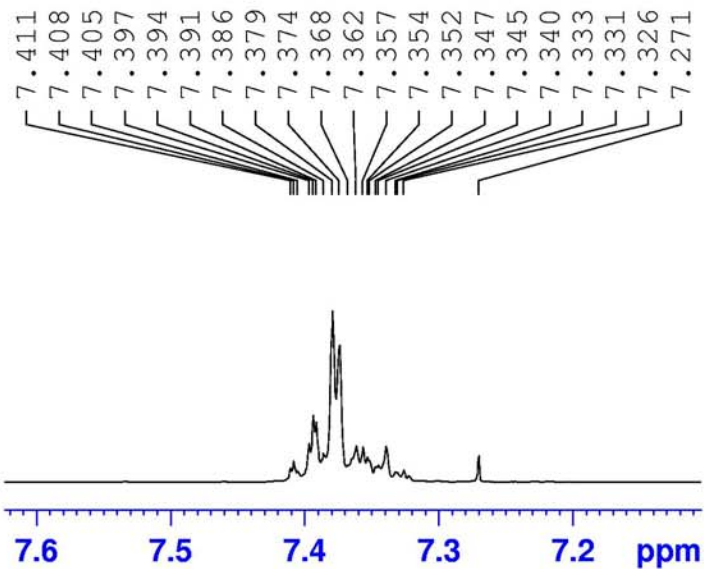

F2 - Acquisition Parameters  
 Date\_ 20070427  
 Time 13.08  
 INSTRUM spect  
 PROBHD 5 mm Multinucl  
 PULPROG zg  
 TD 65536  
 SOLVENT CDC13  
 NS 8  
 DS 2  
 SWH 10330.578 Hz  
 FIDRES 0.157632 Hz  
 AQ 3.1719923 sec  
 RG 32  
 DW 48.400 usec  
 DE 6.00 usec  
 TE 298.2 K  
 D1 10.00000000 sec  
 TD0 1

===== CHANNEL f1 =====  
 NUC1 1H  
 P1 9.00 usec  
 PL1 0.00 dB  
 SFO1 500.1330885 MHz

F2 - Processing parameters  
 SI 32768  
 SF 500.1300079 MHz  
 WDW EM  
 SSB 0  
 LB 0.10 Hz  
 GB 0  
 PC 1.00

