
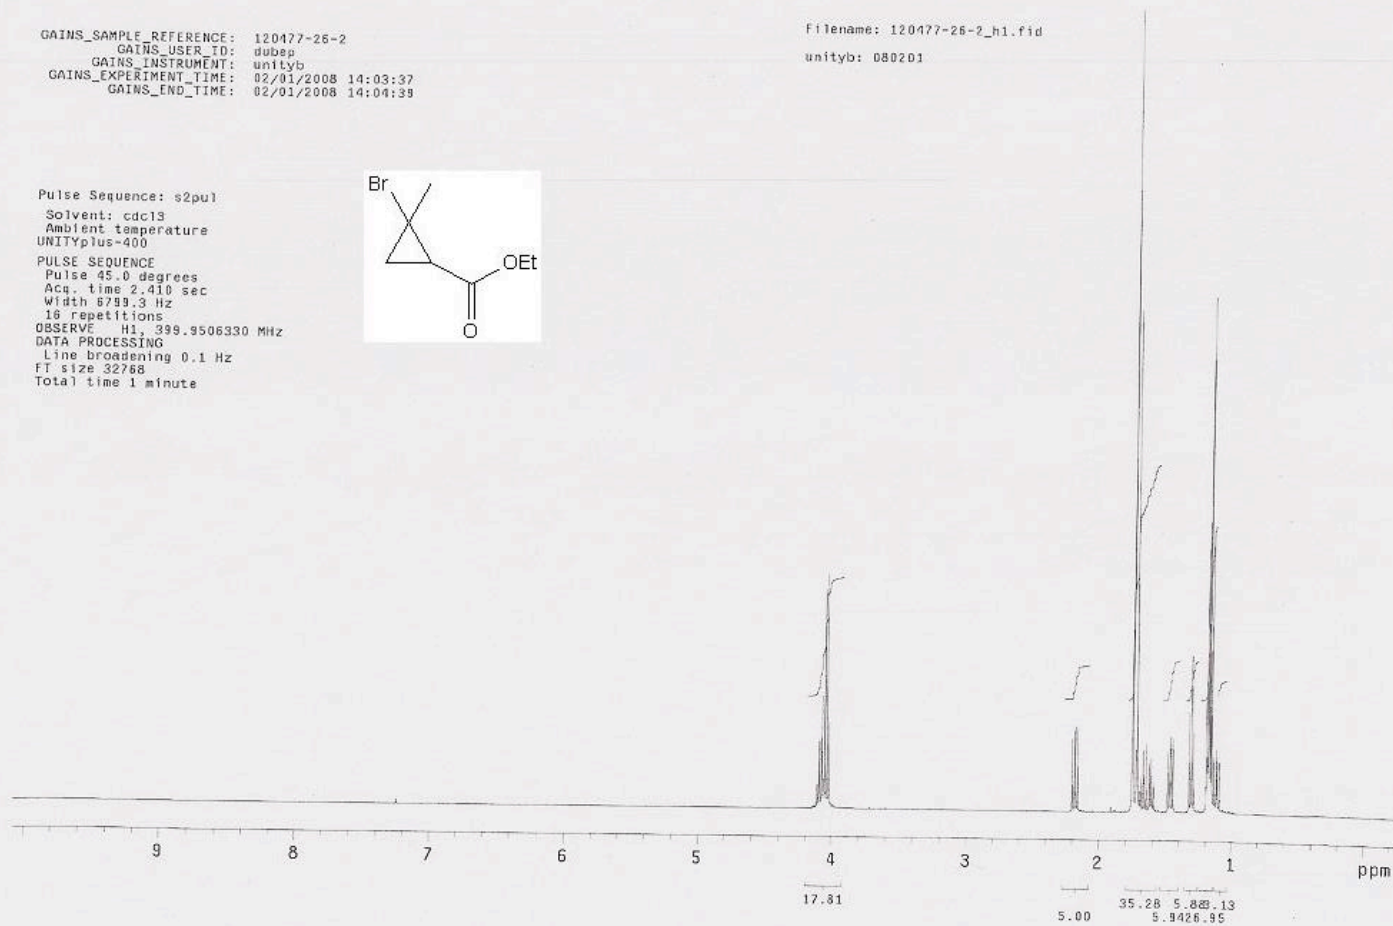


GAINS\_SAMPLE\_REFERENCE: 120477-26-2  
GAINS\_USER\_ID: ddbep  
GAINS\_INSTRUMENT: unityb  
GAINS\_EXPERIMENT\_TIME: 02/01/2008 14:03:37  
GAINS\_END\_TIME: 02/01/2008 14:04:39

Filename: 120477-26-2\_h1.fid

unityb: 080201

Pulse Sequence: s2pul  
Solvent: cdc13  
Ambient temperature  
UNITYplus-400  
PULSE SEQUENCE  
Pulse 45.0 degrees  
Acq. time 2.410 sec  
Width 6799.3 Hz  
16 repetitions  
OBSERVE H1: 399.9506330 MHz  
DATA PROCESSING  
Line broadening 0.1 Hz  
FT size 32768  
Total time 1 minute




DATA\_SAMPLE\_REFERENCE= 120477-20-2

Filename: 120477-20-2\_h1.Fid

unity: 0.00201

INDEX	FREQUENCY	PPM	HEIGHT	INDEX	FREQUENCY	PPM	HEIGHT
1	1344.883	4.119	4.2	35	470.480	1.176	51.8
2	1642.868	4.108	4.5	37	467.158	1.168	32.0
3	1637.327	4.095	12.1	38	463.524	1.159	28.6
4	1635.852	4.090	11.5	39	460.104	1.150	47.8
5	1590.872	4.078	12.9	40	453.454	1.134	9.9
6	1626.382	4.071	20.1	41	447.235	1.118	11.3
7	1625.052	4.053	2.9	42	444.748	1.112	8.2
8	1823.017	4.050	5.2	43	436.938	1.097	9.1
9	1820.912	4.053	39.0				
10	1518.006	4.046	3.0				
11	1613.855	4.035	41.8				
12	1606.801	4.017	15.3				
13	879.688	2.199	12.9				
14	872.633	2.182	14.4				
15	870.143	2.176	15.3				
16	863.502	2.159	14.0				
17	899.570	1.748	151.2				
18	888.364	1.721	89.3				
19	879.648	1.699	3.9				
20	675.499	1.686	5.3				
21	668.859	1.672	11.1				
22	657.198	1.668	6.5				
23	563.558	1.652	12.2				
24	651.428	1.628	8.8				
25	645.202	1.613	9.0				
26	638.582	1.597	5.4				
27	595.816	1.490	10.8				
28	583.175	1.473	13.7				
29	586.270	1.466	11.4				
30	580.045	1.450	13.5				
31	536.742	1.325	17.9				
32	523.502	1.309	27.9				
33	516.962	1.293	14.4				
34	477.950	1.195	27.3				
35	474.630	1.187	48.9				



Step A <sup>1</sup>H peak peaking