



cdt-6-18

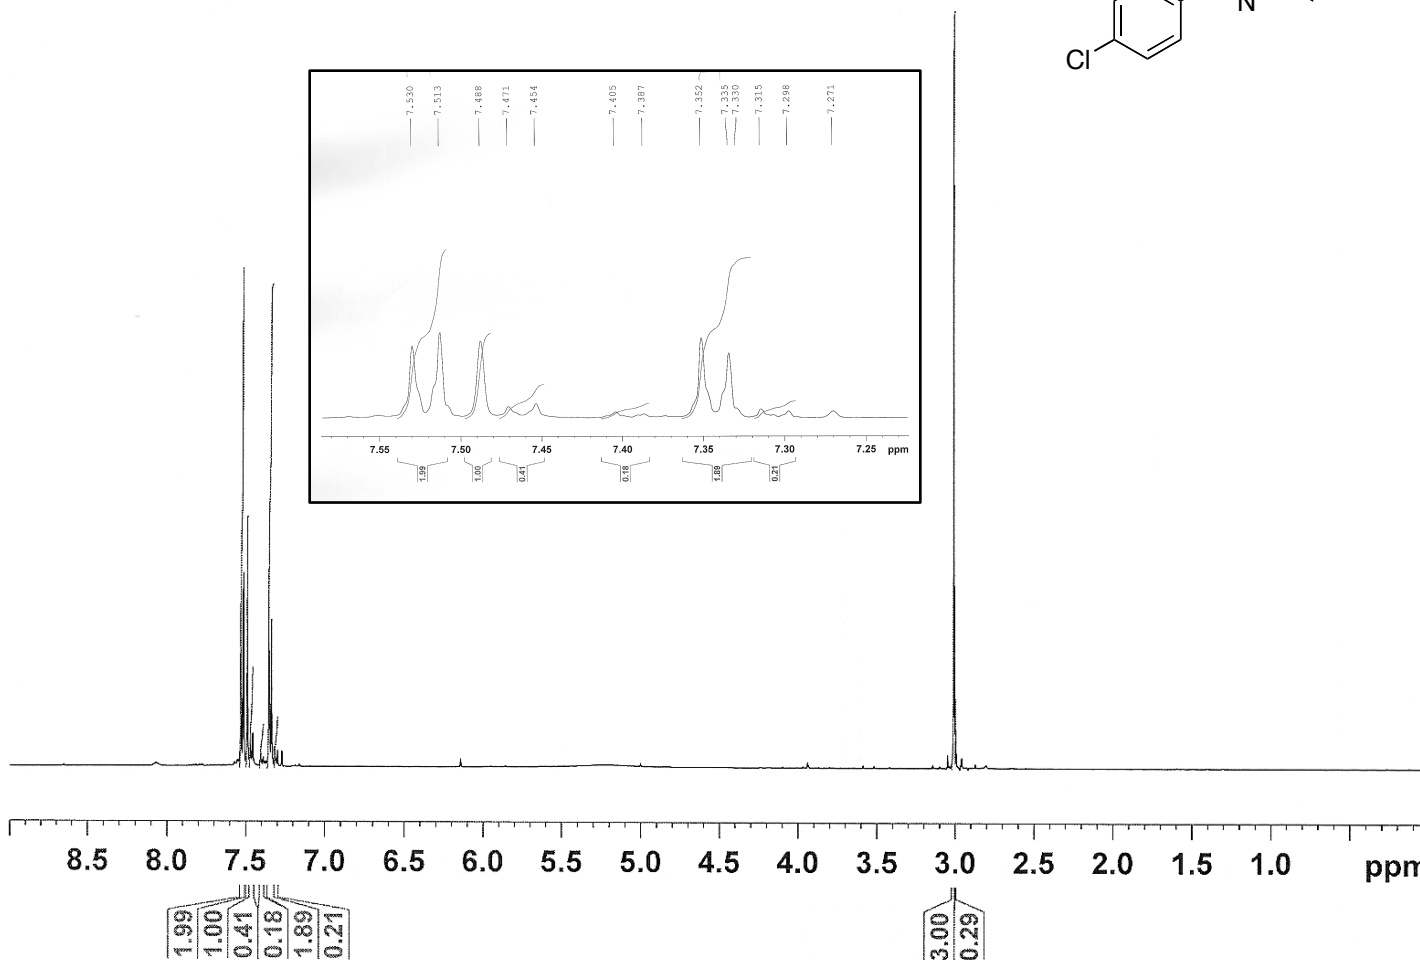

7.530  
7.513  
7.488  
7.471  
7.454  
7.405  
7.387  
7.352  
7.335  
7.330  
7.315  
7.298  
7.271

3.051  
3.011  
3.001  
2.960



Current Data Parameters  
NAME cdt-6-18  
EXPNO 3  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20070815  
Time 17.47  
INSTRUM spect  
PROBHD 5 mm Multinucl  
PULPROG zg  
TD 65536  
SOLVENT CDCl3  
NS 4  
DS 2  
SWH 10330.578 Hz  
FIDRES 0.157632 Hz  
AQ 3.1719923 sec  
RG 16  
DW 48.400 usec  
DE 6.00 usec  
TE 296.2 K  
D1 20.00000000 sec  
TDO 1

==== CHANNEL f1 =====  
NUC1 1H  
P1 9.00 usec  
PL1 0.00 dB  
SFO1 500.1330885 MHz

F2 - Processing parameters  
SI 32768  
SF 500.1299900 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00