
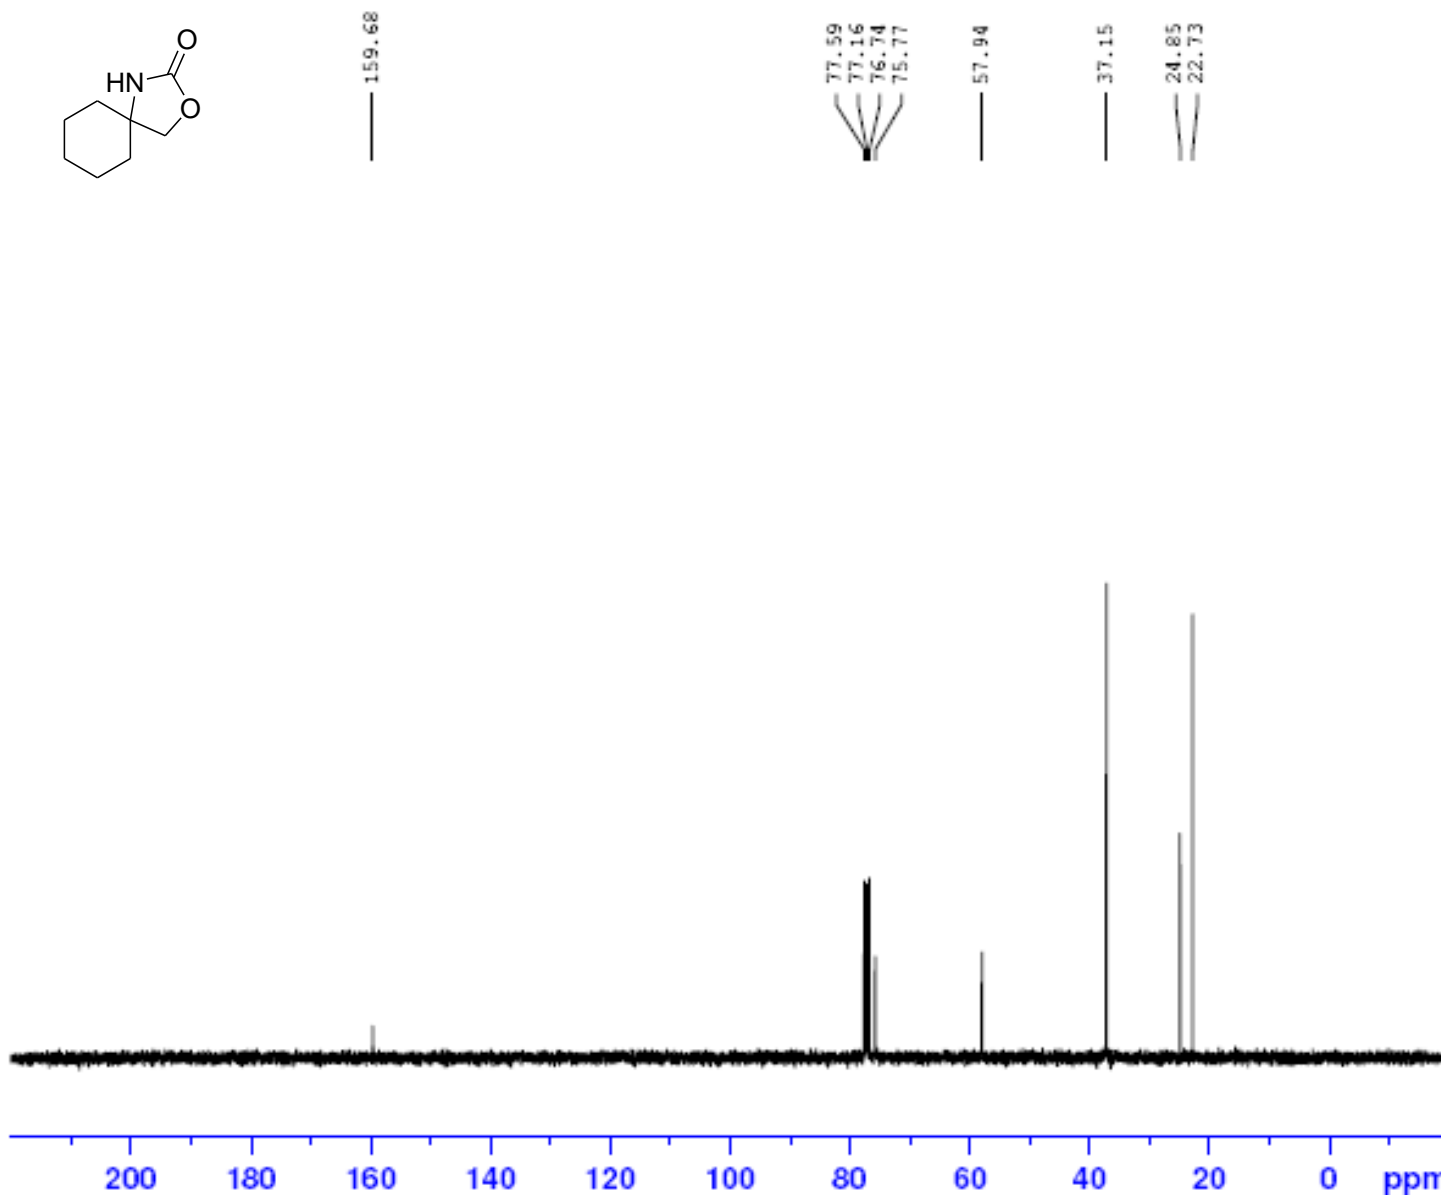


AJR-4-36
NMR 300
OrgSyn Final



Current Data Parameters
NAME AJR-4-36
EXPNO 2
PROCNO 1

F2 - Acquisition Parameters
Date_ 20080626
Time 19.47
INSTRUM spect
PROBHD 5 mm DUL 1H-13
PULPROG zgpg
TD 65536
SOLVENT CDCl3
NS 21
DS 4
SWH 18115.941 Hz
FIDRES 0.276427 Hz
AQ 1.8088436 sec
RG 8192
DW 27.600 usec
DE 6.00 usec
TE 300.0 K
D1 8.00000000 sec
d11 0.03000000 sec
DELTA 7.90000010 sec
TD0 1

==== CHANNEL f1 =====
NUC1 13C
P1 9.00 usec
PL1 1.80 dB
SFO1 75.5381641 MHz

==== CHANNEL f2 =====
CPDPRG2 waltz16
NUC2 1H
PCPD2 92.00 usec
PL2 0.00 dB
PL12 20.00 dB
PL13 20.00 dB
SFO2 300.3812015 MHz

F2 - Processing parameters
SI 65536
SF 75.5306024 MHz
NDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40