


Solvent:  $\text{cdcl}_3$   
 Temp. 25.0 C / 298.1 K  
 UNITYplus-400  
 PULSE SEQUENCE  
 Pulse 45.0 degrees  
 Acq. time 2.411 sec  
 Width 6795.8 Hz  
 16 repetitions  
 OBSERVE H1, 399.7467396 MHz  
 DATA PROCESSING  
 FT size 32768  
 Total time 1 minute

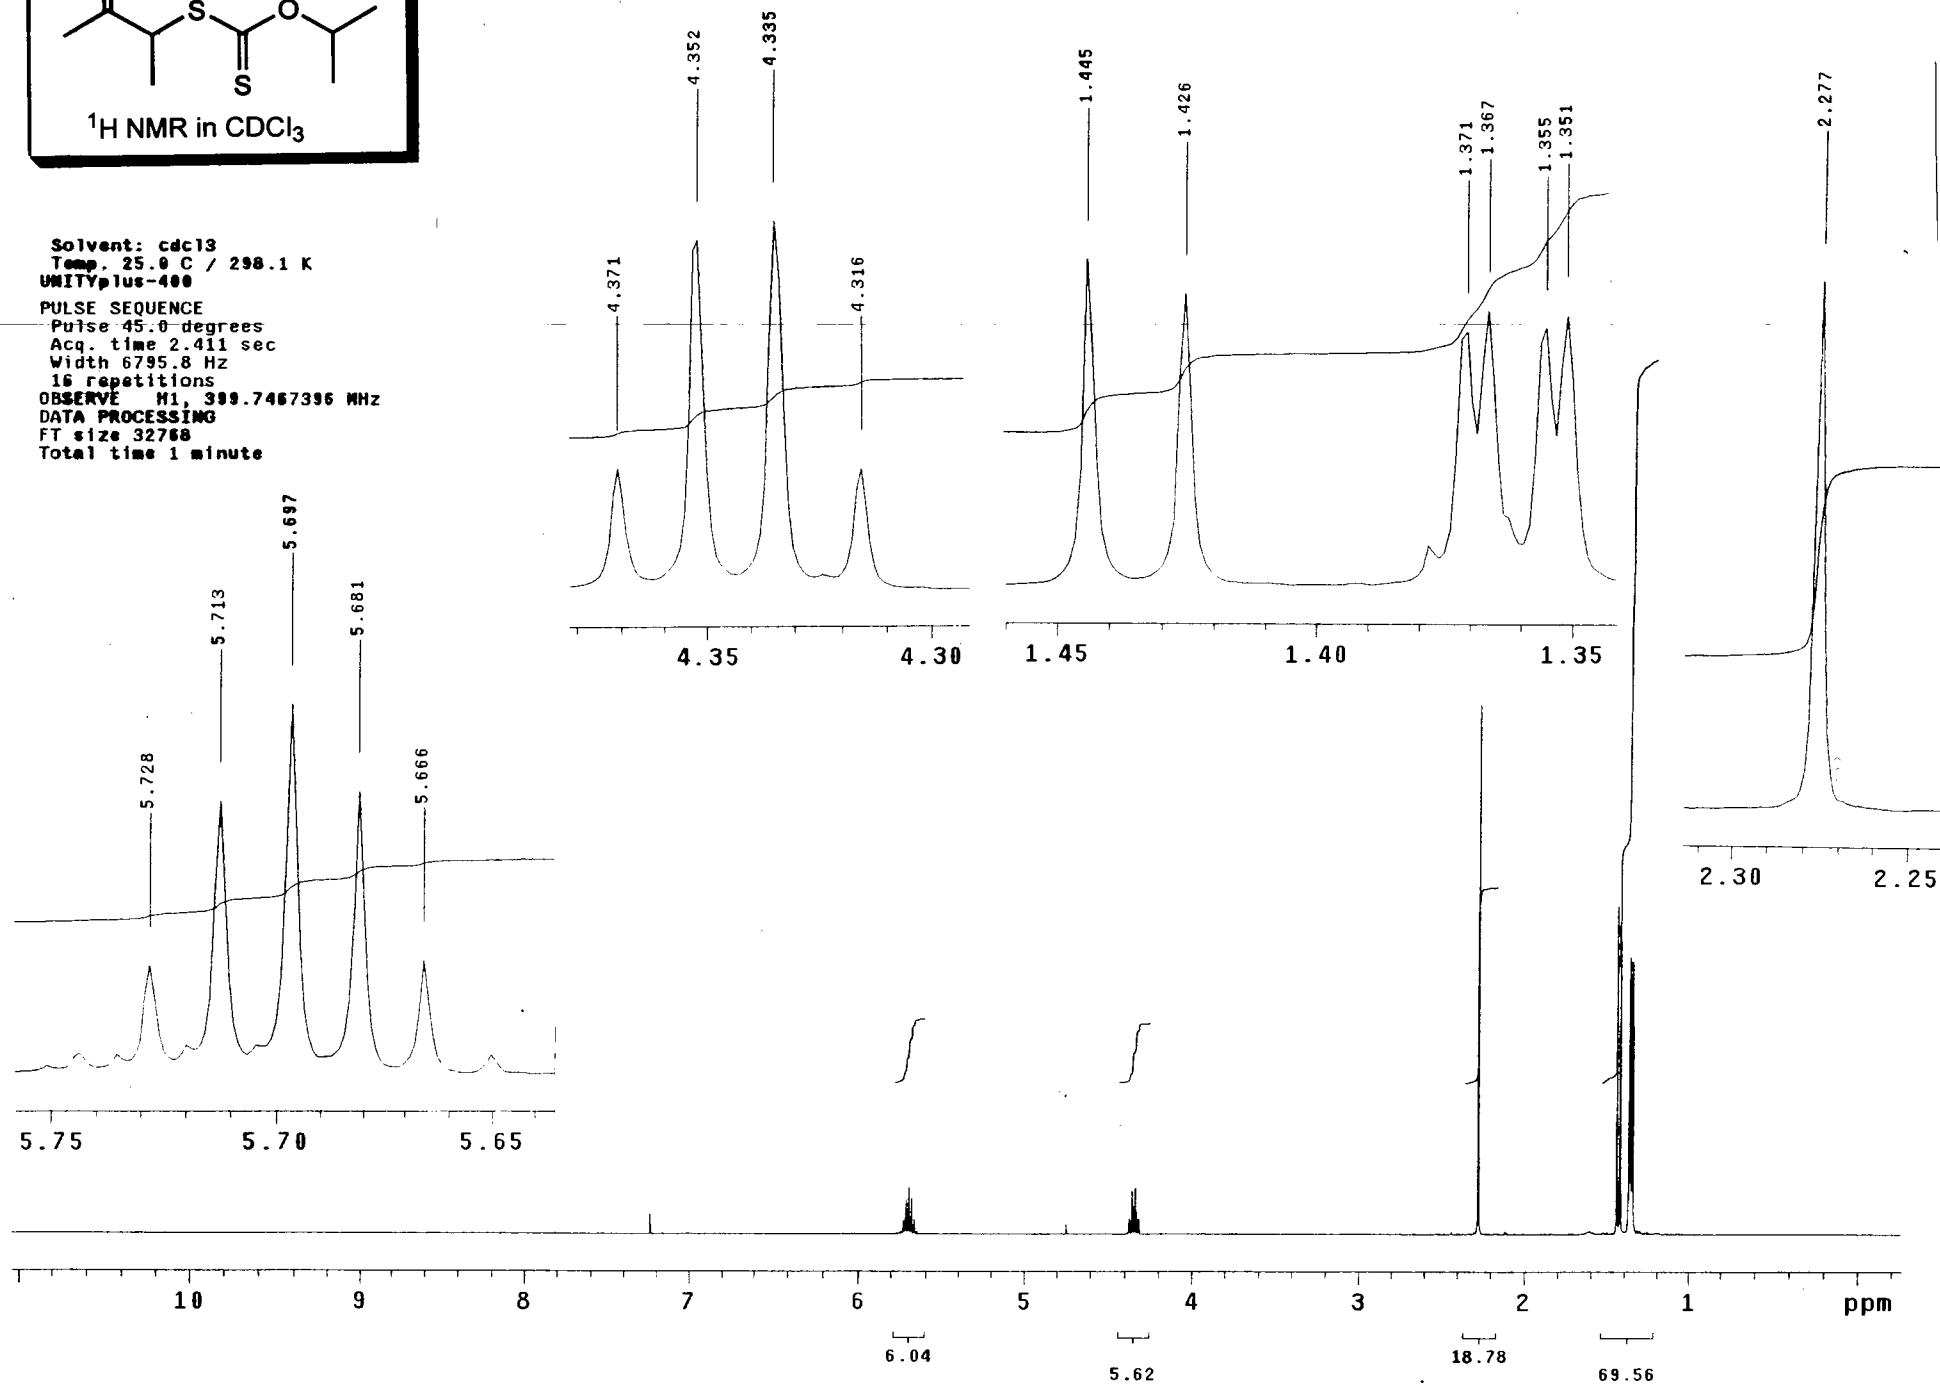

step A distillate

Data not saved (unable to retrieve from ISIS or NMR workstation)

prd400: 090519

INDEX	FREQUENCY	PPM	HEIGHT
1	2894.166	7.240	2.6
2	2283.570	5.713	4.5
3	2277.348	5.697	6.1
4	2271.126	5.681	4.6
5	1747.224	4.371	2.0
6	1739.758	4.352	5.8
7	1732.706	4.335	6.1
8	910.143	2.277	69.8
9	577.468	1.445	43.1
10	570.002	1.426	38.7
11	550.920	1.378	5.5
12	548.017	1.371	33.7
13	546.358	1.367	36.4
14	541.795	1.355	34.2
15	540.135	1.351	35.8