
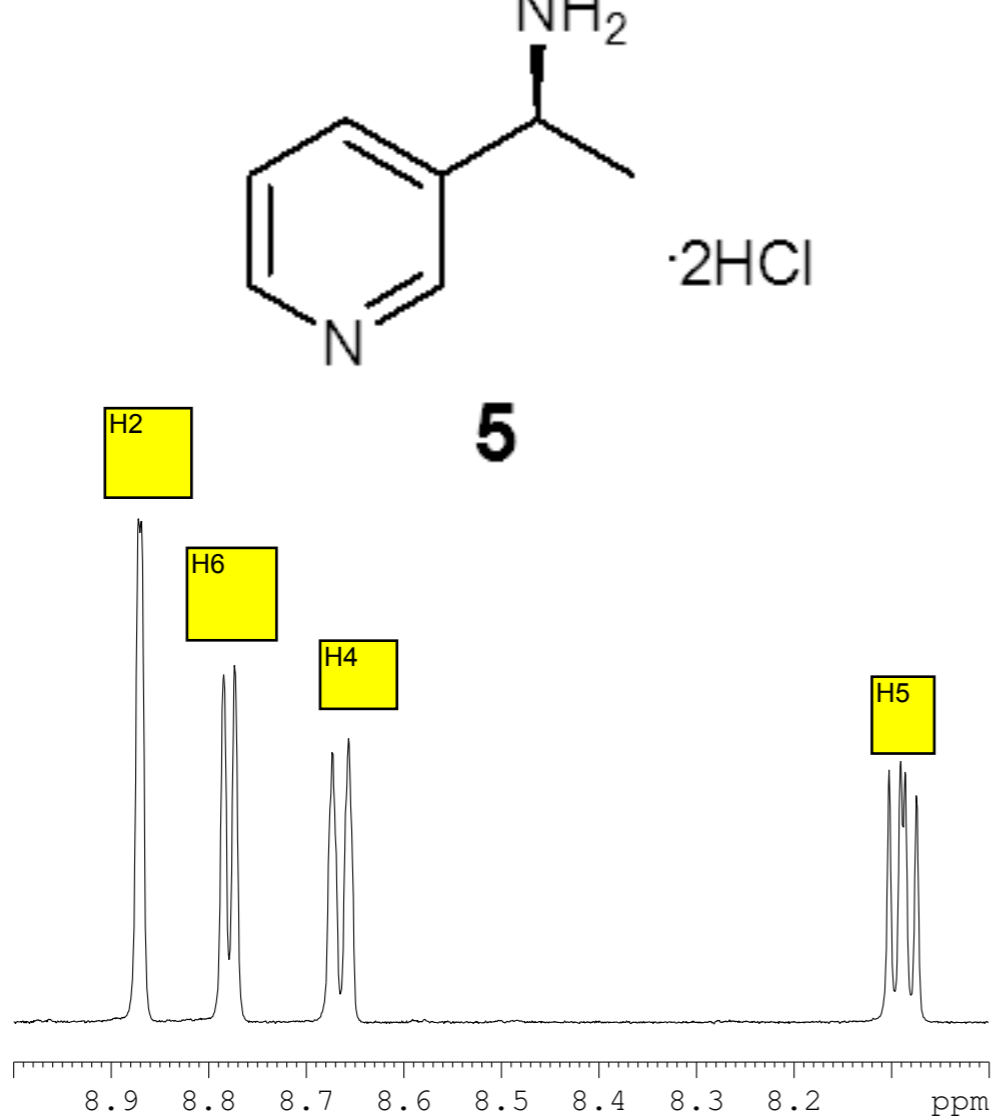


Current Data Parameters  
 NAME 2009-060  
 EXPNO 1  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20090711  
 Time 13.50  
 INSTRUM spect  
 PROBHD 5 mm PABBI 1H-  
 PULPROG zg30  
 TD 65536  
 SOLVENT D2O  
 NS 32  
 DS 4  
 SWH 13020.833 Hz  
 FIDRES 0.198682 Hz  
 AQ 2.5166707 sec  
 RG 1024  
 DW 38.400 usec  
 DE 6.50 usec  
 TE 295.0 K  
 D1 0.10000000 sec  
 TD0 1

==== CHANNEL f1 =====  
 NUC1 1H  
 P1 8.60 usec  
 PL1 -1.00 dB  
 SFO1 500.3330895 MHz

F2 - Processing parameters  
 SI 32768  
 SF 500.3300000 MHz  
 WDW no  
 SSB 0  
 LB 0.00 Hz  
 GB 0  
 PC 1.00

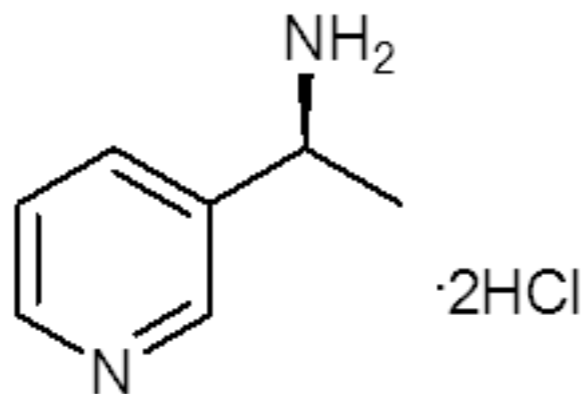

Peak	?(F1) [ppm]	?(F1) [Hz]	Intensity	Annotation
1	8.8716	4438.7276	4.30	
2	8.8689	4437.3767	4.32	
3	8.7846	4395.1989	2.97	
4	8.7731	4389.4451	3.04	
5	8.6728	4339.2620	2.32	
6	8.6563	4331.0066	2.43	
7	8.1023	4053.8238	2.16	
8	8.0905	4047.9199	2.25	
9	8.0859	4045.6183	2.16	
10	8.0742	4039.7645	1.94	
11	4.8148	2408.9889	0.94	
12	4.8009	2402.0343	2.94	
13	4.7870	2395.0797	2.97	
14	4.7730	2388.0751	0.97	
15	4.7003	2351.7011	40.00	
16	1.6693	835.2009	13.28	
17	1.6553	828.1962	13.15	

