


CDC13 + TMS, 500MHz

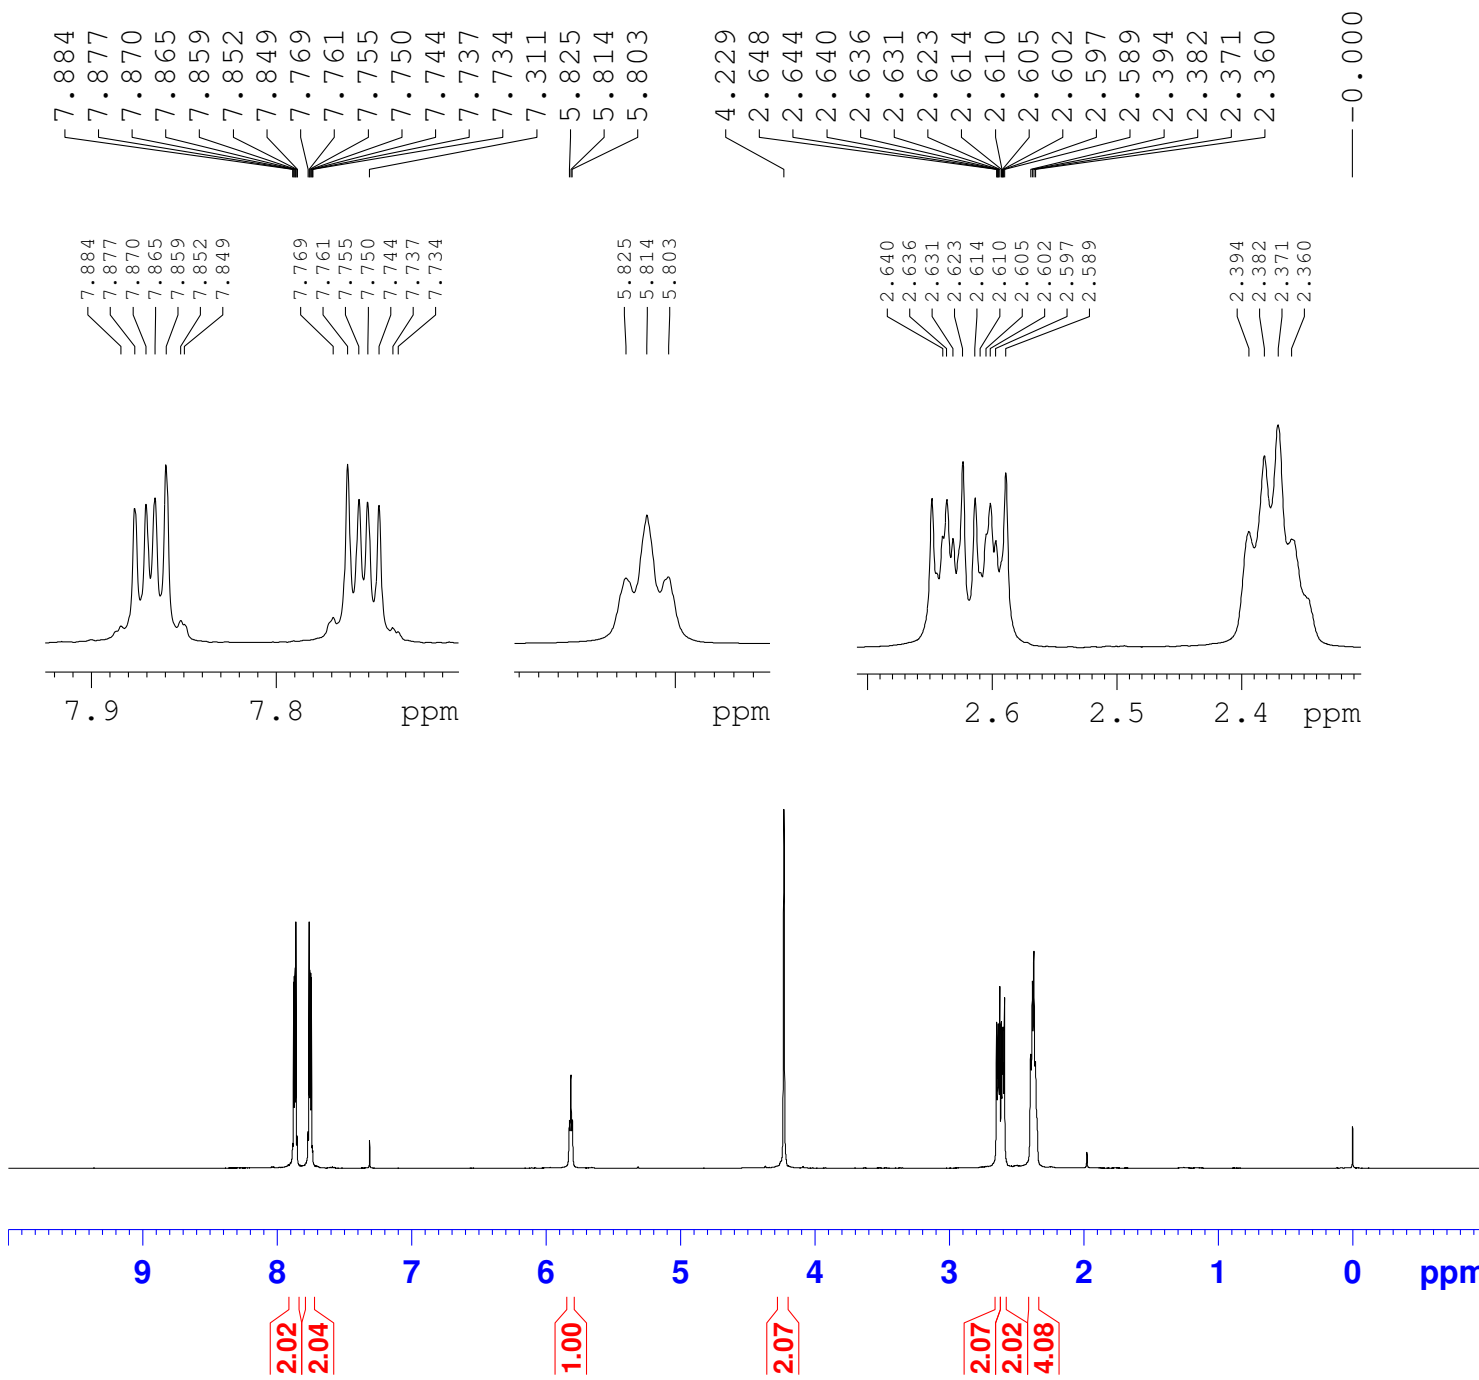

Current Data Parameters  
NAME JMO6-154  
EXPNO 3  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20101018  
Time 14.31  
INSTRUM spect  
PROBHD 5 mm PABBO BB-  
PULPROG zg30  
TD 65536  
SOLVENT CDC13  
NS 8  
DS 2  
SWH 10330.578 Hz  
FIDRES 0.157632 Hz  
AQ 3.1719923 sec  
RG 32  
DW 48.400 usec  
DE 6.50 usec  
TE 293.7 K  
D1 2.00000000 sec

==== CHANNEL f1 =====  
NUC1 1H  
P1 10.20 usec  
PLW1 18.74300003 W  
SFO1 500.1630887 MHz

F2 - Processing parameters  
SI 65536  
SF 500.1599854 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00