



142.93  
141.60  
129.58  
125.37

81.92  
77.25  
77.00  
76.75  
74.42  
61.95

23.73  
21.50



Fast diastereomer on TLC

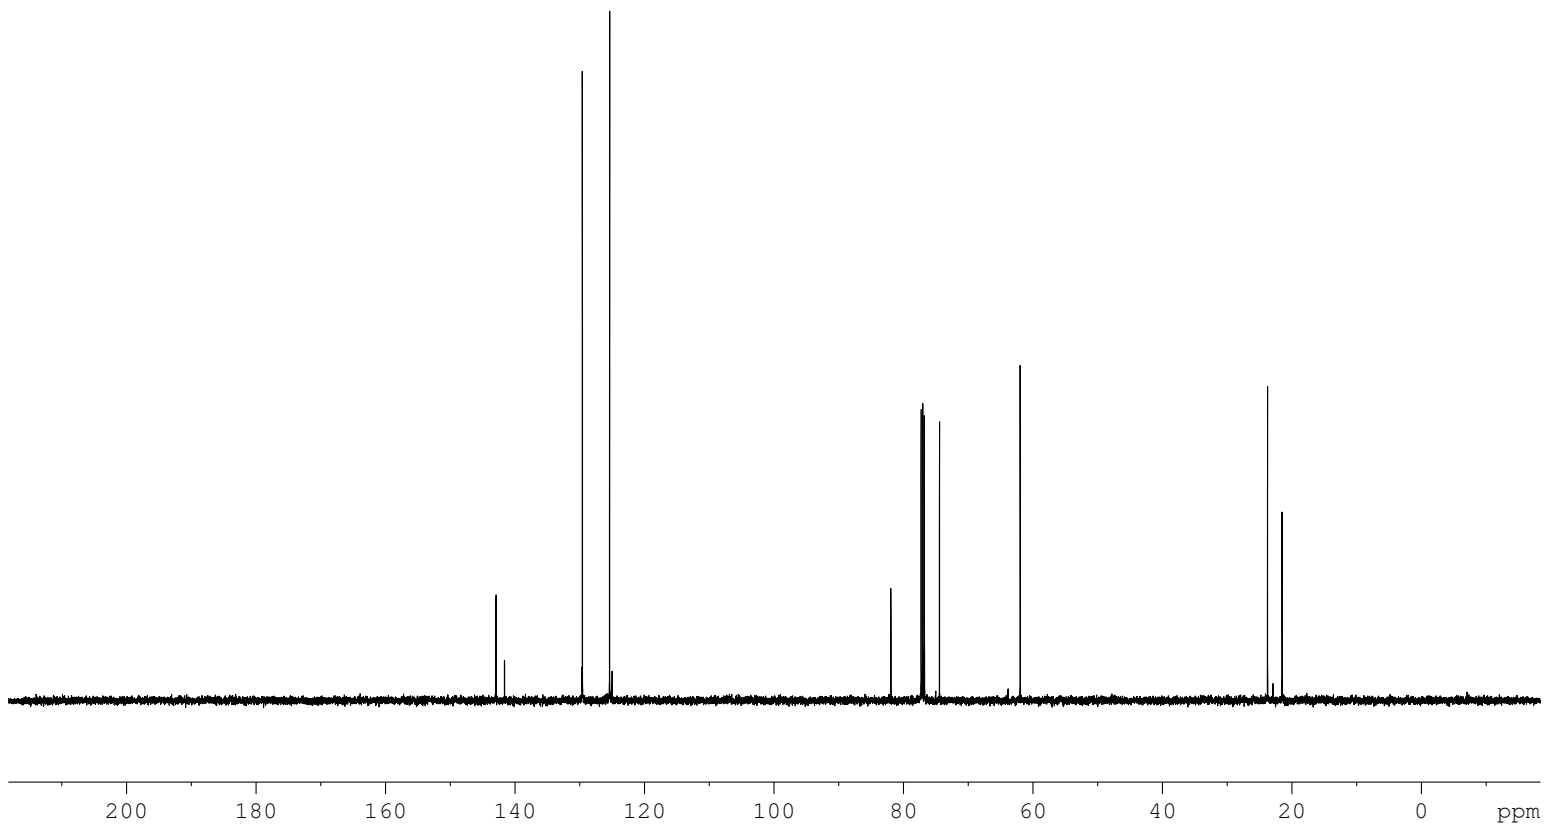

Current Data Parameters  
NAME BW001  
EXPNO 2  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20110121  
Time 16.18  
INSTRUM spect  
PROBHD 5 mm PABBO BB-  
PULPROG zgpg30  
TD 65536  
SOLVENT CDC13  
NS 85  
DS 4  
SWH 29761.904 Hz  
FIDRES 0.454131 Hz  
AQ 1.1010548 sec  
RG 203  
DW 16.800 usec  
DE 6.50 usec  
TE 293.9 K  
D1 2.00000000 sec  
D11 0.03000000 sec

==== CHANNEL f1 =====  
NUC1 13C  
P1 8.80 usec  
PLW1 112.58000183 W  
SFO1 125.7779080 MHz

==== CHANNEL f2 =====  
CPDPRG2 waltz16  
NUC2 1H  
PCPD2 80.00 usec  
PLW2 18.74300003 W  
PLW12 0.36736000 W  
PLW13 0.18408000 W  
SFO2 500.1620006 MHz

F2 - Processing parameters  
SI 32768  
SF 125.7653388 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40