


7.646
7.630
7.346
7.330
7.260



5.043
5.039
5.030
5.026
5.017
5.013
5.003
4.999

2.642
2.637
2.424

1.532
1.518



slow diastereomer on TLC

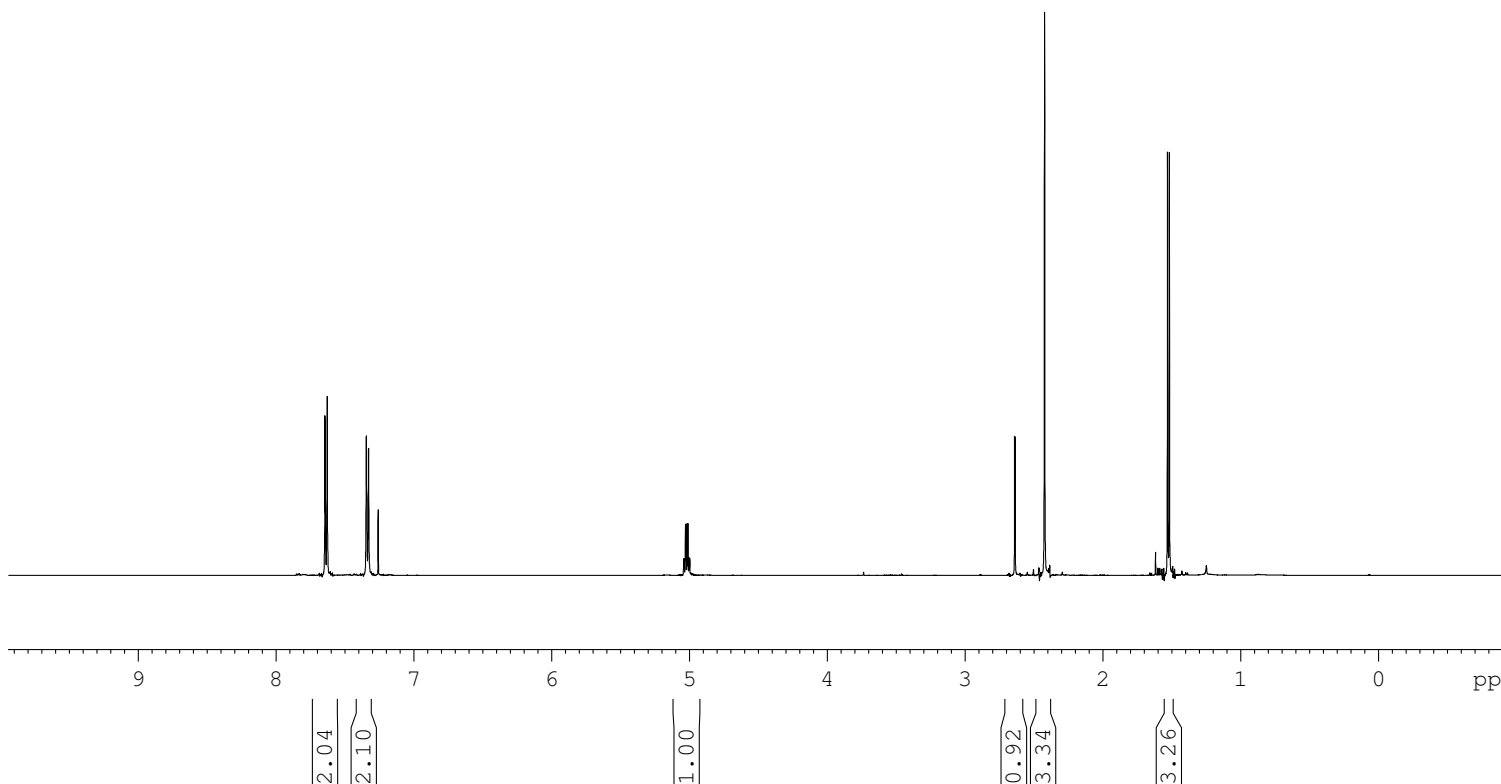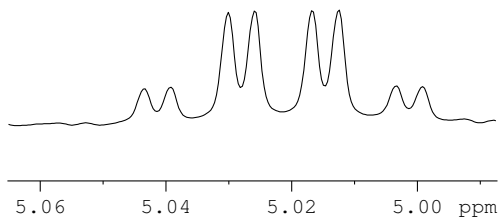

2.04
2.10

1.00

0.92
3.34

3.26

Current Data Parameters
NAME BW001-2
EXPNO 1
PROCNO 1

F2 - Acquisition Parameter.
Date_ 20110121
Time 16.34
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 10330.578 Hz
FIDRES 0.157632 Hz
AQ 3.1719923 se
RG 71.8
DW 48.400 us
DE 6.50 us
TE 293.7 K
D1 1.00000000 se

===== CHANNEL f1 =====
NUC1 1H
P1 10.20 us
PLW1 18.74300003 W
SFO1 500.1630887 MH

F2 - Processing parameters
SI 65536
SF 500.1600113 MH
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00