

—207.95

1,5-Dioxaspiro[5.5]undecan-3-one


—99.83

—66.48

—32.49

—25.17

—22.75

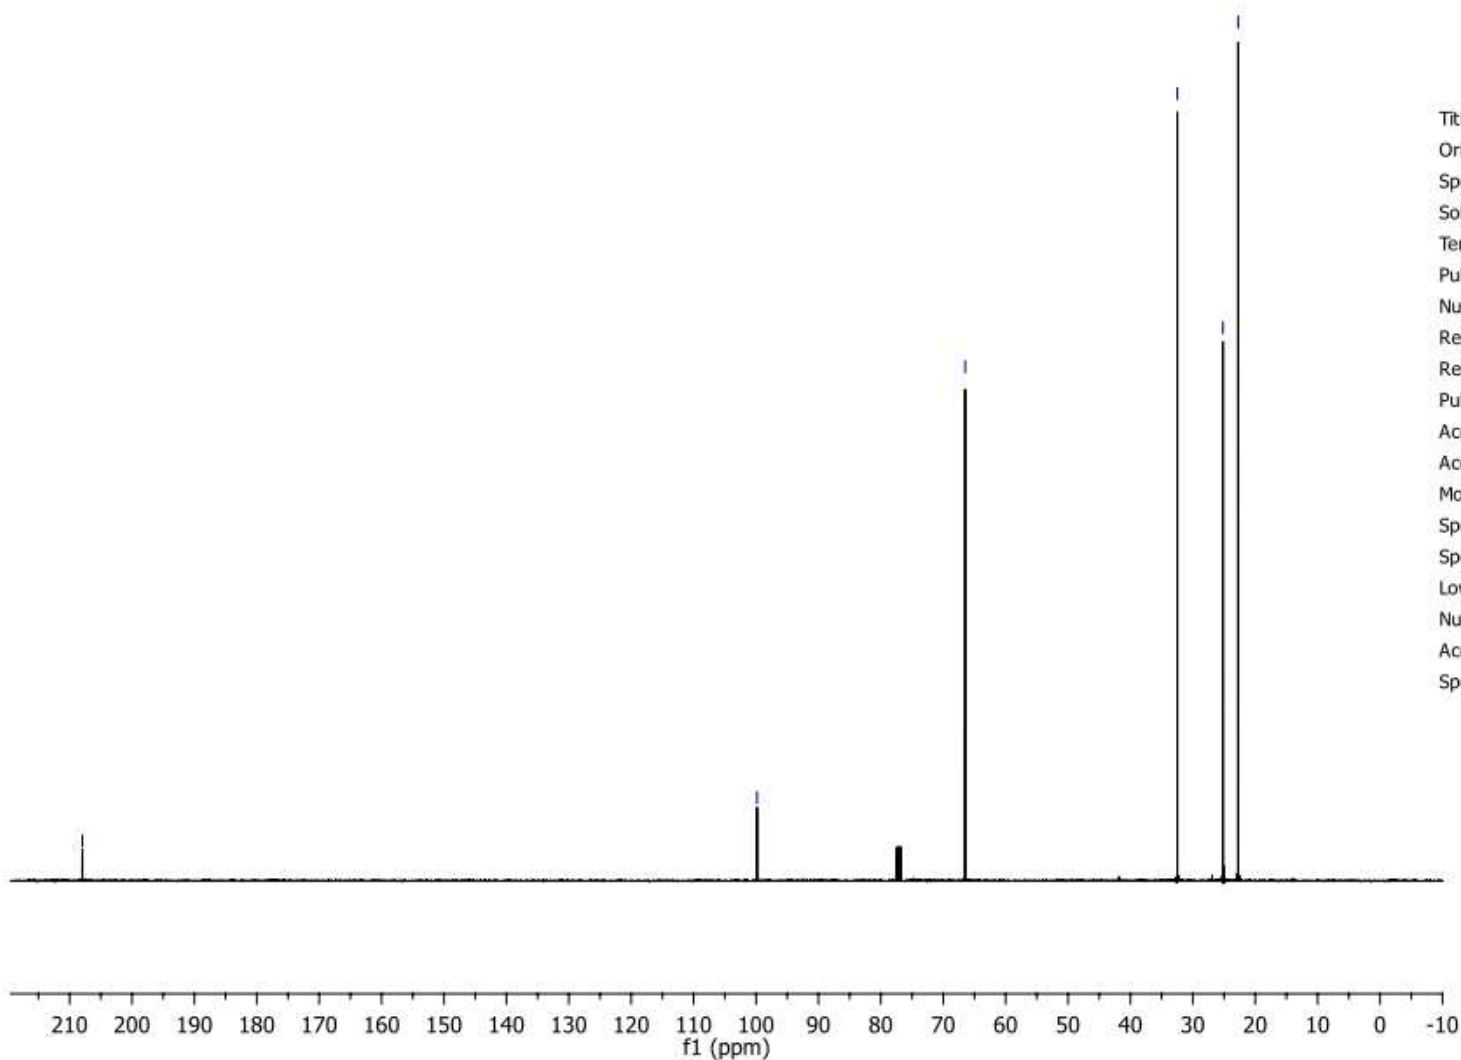

Title	MW-1-140 13C
Origin	Bruker BioSpin GmbH
Spectrometer	spect
Solvent	CDCl3
Temperature	298.1
Pulse Sequence	zgpg30
Number of Scans	146
Receiver Gain	203
Relaxation Delay	2.0000
Pulse Width	10.0000
Acquisition Time	1.3631
Acquisition Date	2016-02-27T21:26:27
Modification Date	2016-02-27T21:26:37
Spectrometer Frequency	100.61
Spectral Width	24038.5
Lowest Frequency	-1958.3
Nucleus	13C
Acquired Size	32768
Spectral Size	65536