



JCL1-00022

8.05  
8.03  
8.02  
8.01  
7.99  
7.97  
7.95  
7.94  
7.92  
7.91  
7.87  
7.87  
7.86  
7.27

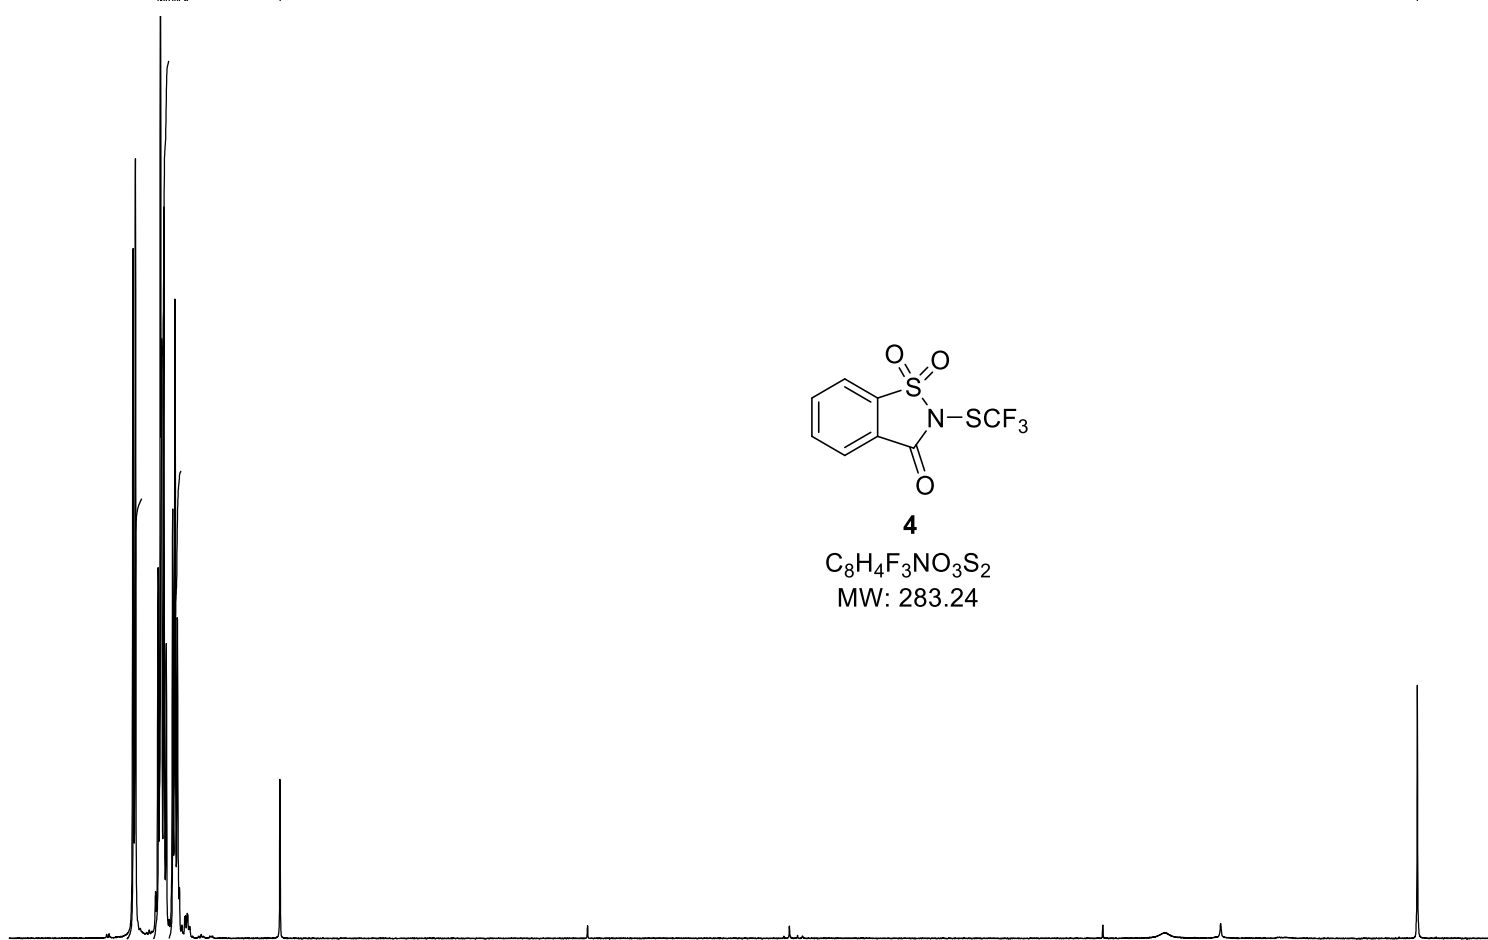

4

C<sub>8</sub>H<sub>4</sub>F<sub>3</sub>NO<sub>3</sub>S<sub>2</sub>  
MW: 283.24



0.00

Current Data Parameters  
NAME jcl1-00022  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20170501  
Time\_ 11.38  
INSTRUM spect  
PROBHD 5 mm PABBO BB-  
PULPROG zg10  
TD 32768  
SOLVENT CDCl3  
NS 16  
DS 0  
SWH 7500.000 Hz  
FIDRES 0.228882 Hz  
AQ 2.1845334 sec  
RG 406  
DW 66.667 usec  
DE 6.50 usec  
TE 299.0 K  
D1 1.00000000 sec  
TD0 1

==== CHANNEL f1 =====  
SFO1 500.1325007 MHz  
NUC1 1H  
P1 11.75 usec  
PLW1 18.39999962 W

F2 - Processing parameters  
SI 16384  
SF 500.1300080 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

1.00  
1.99  
1.06