
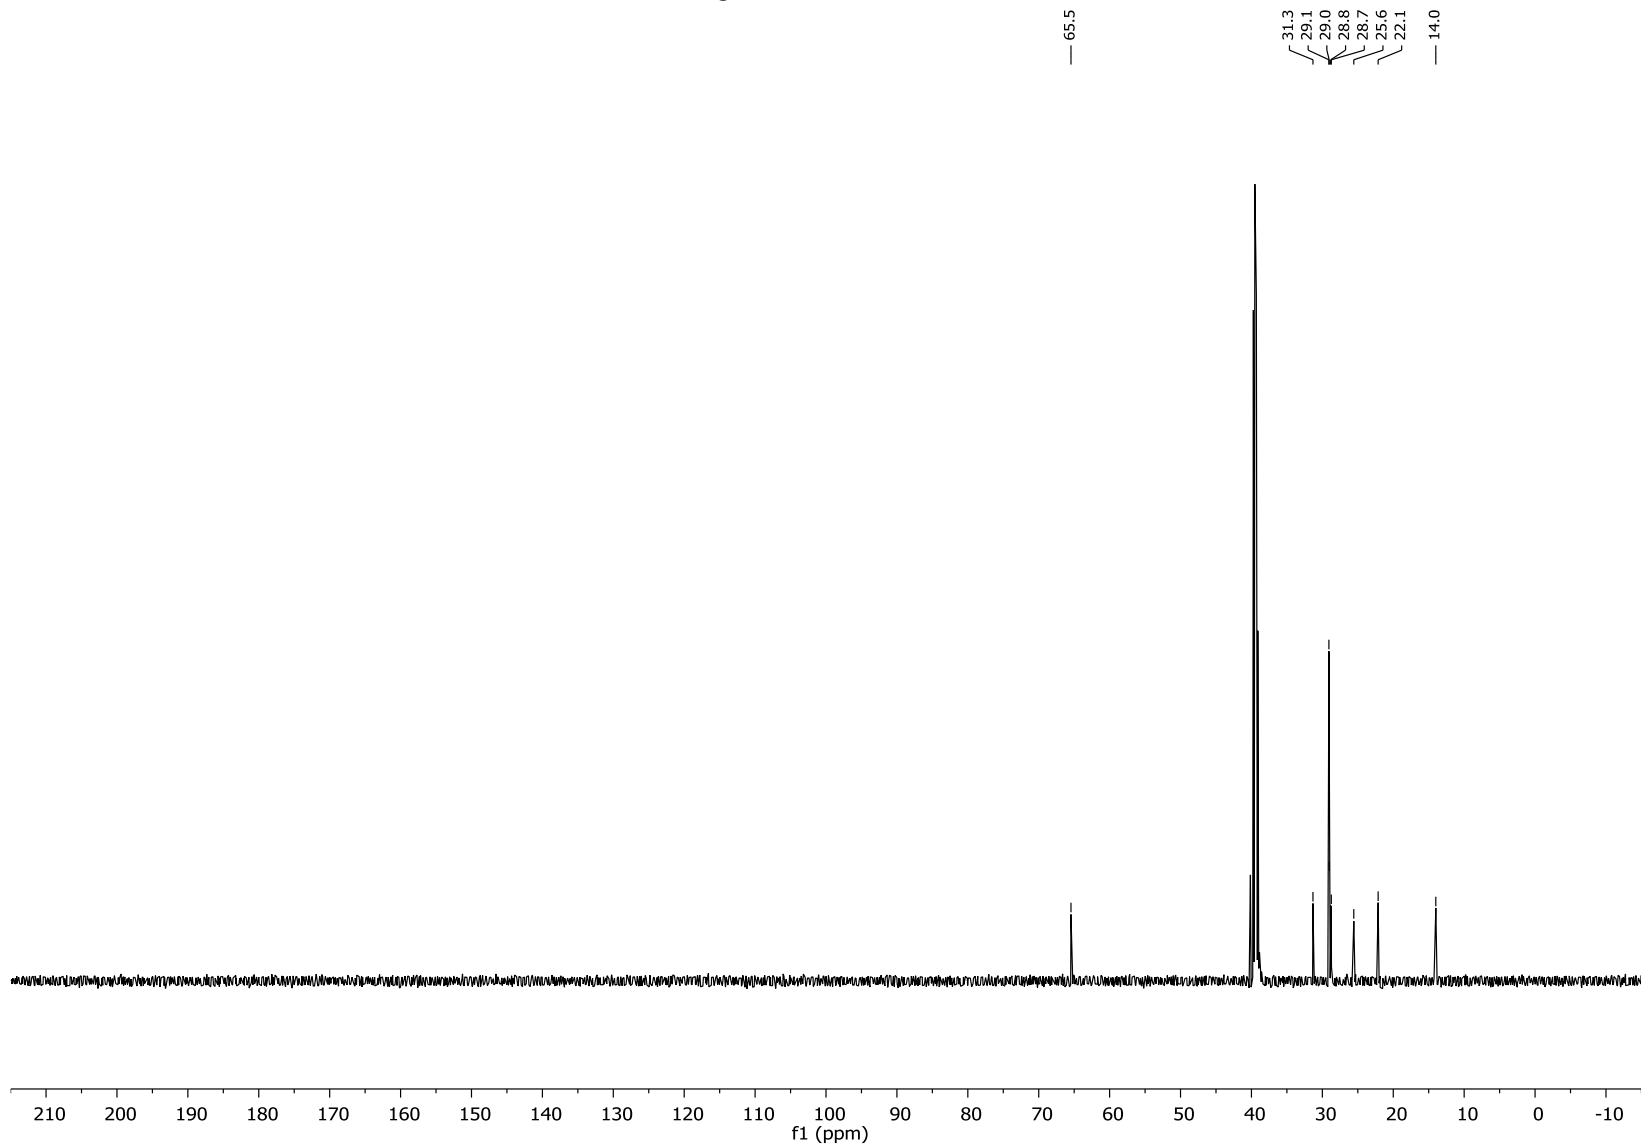


sodium heptadecyl sulfate



Parameter	Value
1 Comment	Sample FXP-IV-001-2 Instrument AV-NEO 400 MHz Group carrei 400 MHz 1H Spectrum
2 Solvent	DMSO
3 Temperature	298.0
4 Pulse Sequence	zgpg45
5 Probe	Z160669_0002 (PA BBO 400S1 BBF-H-D-05 Z SP FB N)
6 Number of Scans	512
7 Receiver Gain	20.3
8 Relaxation Delay	0.3000
9 Pulse Width	10.0000
10 Acquisition Date	2017-10-09T19:25:18
11 Spectrometer Frequency	100.63
12 Spectral Width	23809.5
13 Lowest Frequency	-1888.0
14 Nucleus	13C
15 Acquired Size	49999
16 Spectral Size	131072