
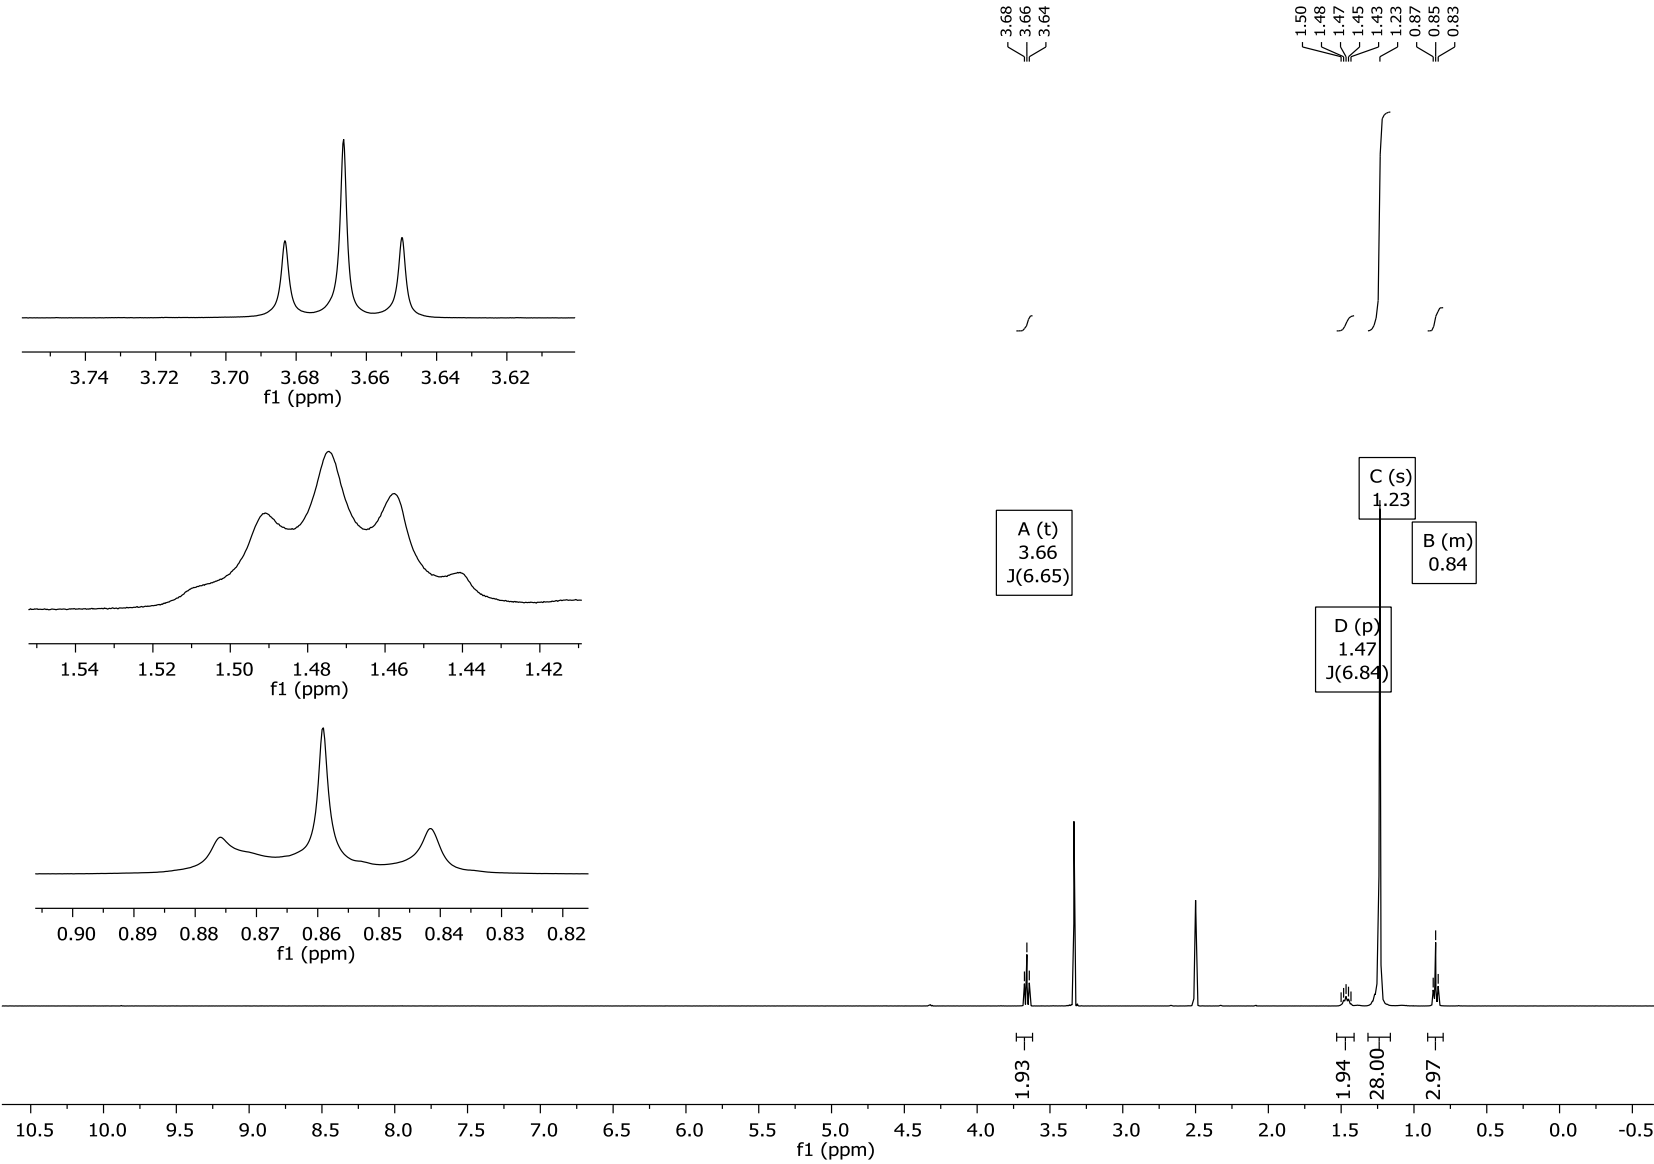


sodium heptadecyl sulfate



Parameter	Value
1 Comment	Sample FXP-IV-001-2 Instrument AV-NEO 400 MHz Group carrei 400 MHz 1H Spectrum
2 Solvent	DMSO
3 Temperature	298.0
4 Pulse Sequence	zg30
5 Probe	Z160669_0002 (PA BBO 400S1 BBF-H-D-05 Z SP FB N)
6 Number of Scans	32
7 Receiver Gain	92.3
8 Relaxation Delay	0.0100
9 Pulse Width	10.0000
10 Acquisition Date	2017-10-09T18:30:38
11 Spectrometer Frequency	400.15
12 Spectral Width	5555.6
13 Lowest Frequency	-376.9
14 Nucleus	1H
15 Acquired Size	27777
16 Spectral Size	65536